

Final Report

Calibration-Round-Robin

CaRo 13

Adolf Kühner AG

Dinkelbergstr. 1
CH-4127 Birsfelden
Switzerland

Tel. +41 (0)61 319 93 93
Fax. +41 (0)61 319 93 94
E-mail office@kuhner.com
Internet www.kuhner.com

This report shall not be published or reproduced other than in full.

CaRo 13	1
1. Conclusion	2
2. Explosion Indices Pmax, Kmax	5
3. Minimum Ignition Energy MIE	7
4. Troubles with chemical igniters	9
5. List of Participants	11

1. Conclusion

According to international standards (e.g. ISO 9000, GLP), test equipment must be calibrated at intervals by comparison with a standard or a calibrated testing apparatus.

This calibration also applies to the 20-l-apparatus and the 1-m³-vessel for the determination of P_{max} and K_{max} and the apparatus for determination of the minimum ignition energy. The test procedure is an important part of this calibration. A general check at the component level is incomplete and hence inadmissible.

Unfortunately there are neither internationally recognized reference samples nor reference equipment available for the determination of these explosion characteristics. Therefore the following calibration method has been carried out successfully:

A dust has been selected, prepared and supplied to **59** test laboratories all over the world. The mean values of the explosion indices, measured by the participating laboratories, has been calculated as reference values. The testing laboratories have been informed about the evaluation with a certificate.

This report presents the results of this calibration method and describes the evaluation procedures. It also demonstrates that with this method it was possible to discover and rectify the cause of any errors with installations producing results differing widely from the reference values.

CaRo 13 - Reference values for the Explosion Indices P_{max} and K_{max}

P_{max} (bar)	8.2 ± 10% (7.4 ... 9.0)
K_{max} (bar·m/s)	253 ± 10% (228 ... 278)

CaRo 13 – Reference values for the Minimum Ignition Energy MIE

Es / 3	Es	Es · 3
0.5 mJ	1.5 mJ	4.5 mJ



Birsfelden, February 2014

Adolf Kühner AG
Christoph Cesana

1.1 Participants

For details see section "list of participants".

	Pmax, Kmax (69)		MZE (53)	
	20-l	1 m ³	MIKE	others
Australia	2		1	
Austria	3		2	
Belgium	2		2	
Canada	1		1	
Czechoslovakia	1		1	
England	3		1	2
France	3		2	
Germany	13	3	18	1
Hungary				1
India			1	
Italy	3		2	
Japan	1		4	
Niederlande	1		1	
Norway	1		1	
Poland	2	1		2
Slovenia	1			
South Africa	1			
Switzerland	3		5	
U.S.A	11		9	1
total:	52	4	51	7

This calibration round robin test „CaRo 13“ has been accepted world wide as the best and most reliable calibration method for this type of test equipment.

1.2 Test substance

For correct calibration the CaRo 13 test sample has been milled, homogenized and shipped in an air tight package. Therefore the sample has to be tested „as delivered“.


CaRo 13 = Niacin USP special (Nicotinic acid)

Particle size:

	d 10	d 50 = median	d 90
Sample 1	4 µm	18 µm	66 µm
Sample 2	5 µm	19 µm	70 µm
Sample 3	4 µm	19 µm	68 µm
Sample 4	4 µm	18 µm	66 µm
Sample 5	5 µm	18 µm	69 µm
Sample 6	4 µm	18 µm	67 µm
Sample 7	4 µm	18 µm	64 µm
Sample 8	5 µm	18 µm	67 µm
Sample 9	5 µm	19 µm	74 µm
Sample 10	4 µm	18 µm	65 µm
Sample 11	4 µm	18 µm	70 µm
Sample 12	4 µm	19 µm	65 µm


2. Explosion Indices Pmax, Kmax

Pmax = 8.2 bar ± 10% (7.4 ... 9.0) by 502 g/m3

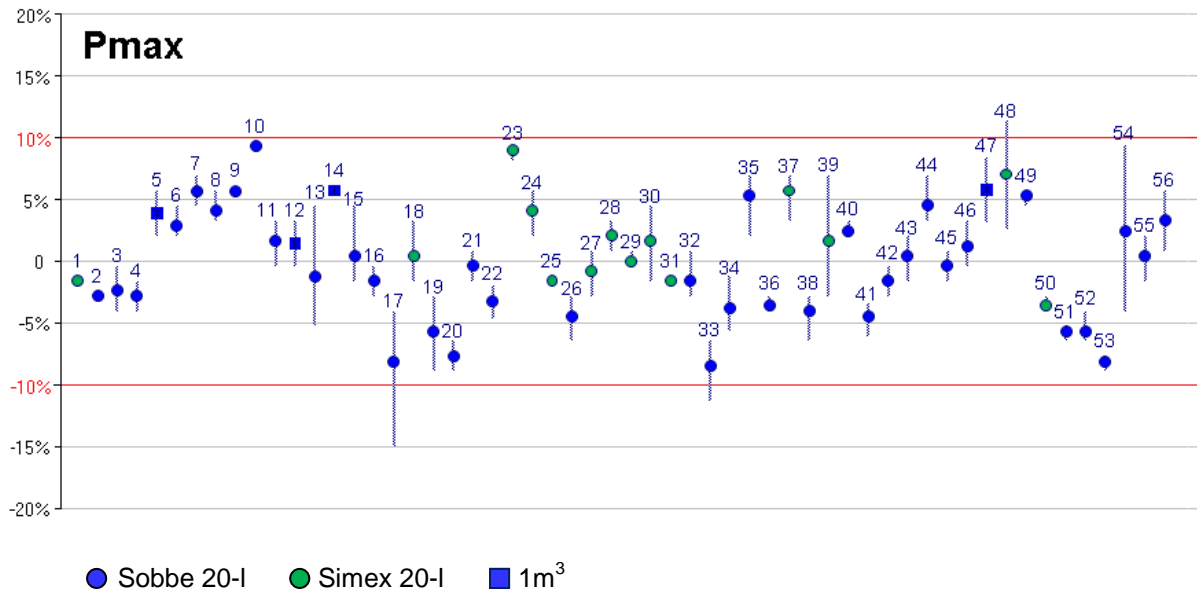

The individual results are drawn in relation to the arithmetic mean of all results and in chronological sequence (number of certificate).

Kmax = 253 bar·m/s ± 10% (228 ... 278) by 622 g/m3

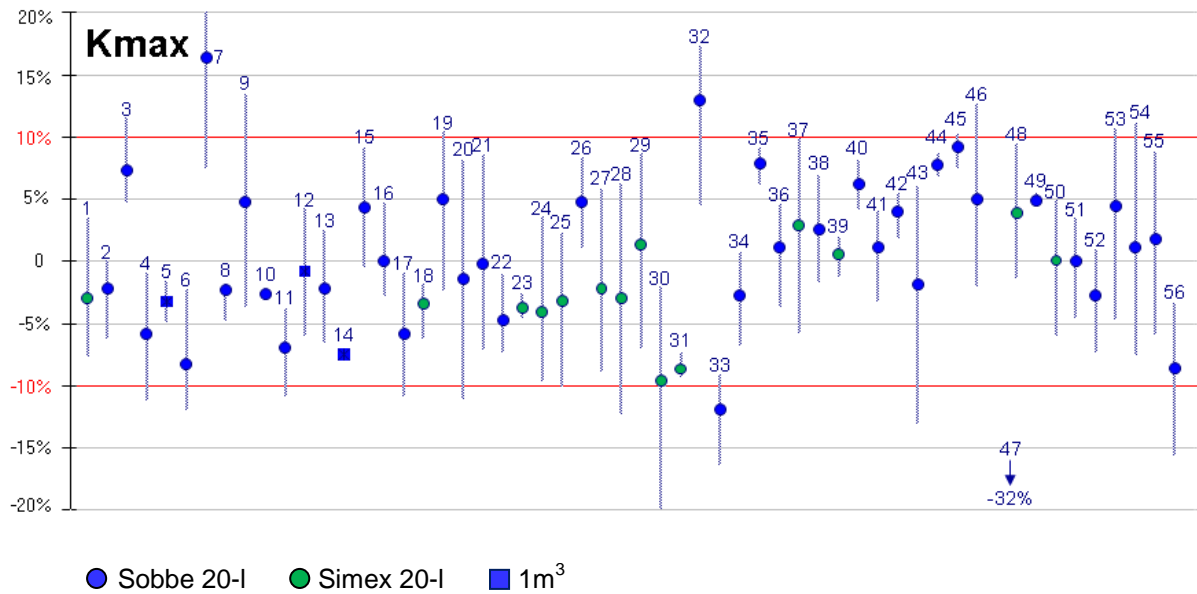

The individual results are drawn in relation to the arithmetic mean of all results and in chronological sequence (number of certificate).

2.1 Test procedure:

The method for determination of Pmax, Kmax is described in the „Manual CaRo 13“.

2.2 Evaluation:

The explosion indices Pmax and (dP/dt)max are defined as the mean values of the maximum values of each series. Subsequently, the explosion index Kmax is calculated from the mean value (dP/dt)max.


2.3 Scatter of Pmax and Kmax:

The maxima of each series must not deviate by more than **10%** of Pmax resp. Kmax. Otherwise this series must be repeated!

2.4 Calculation of the reference values:

First the mean values of all test results (54) has been calculated. In a 2nd step all results outside of the tolerance band are excluded prior to the subsequent calculation of the mean value. Due to the large number of participants the mean values did not change.

3. Minimum Ignition Energy MIE

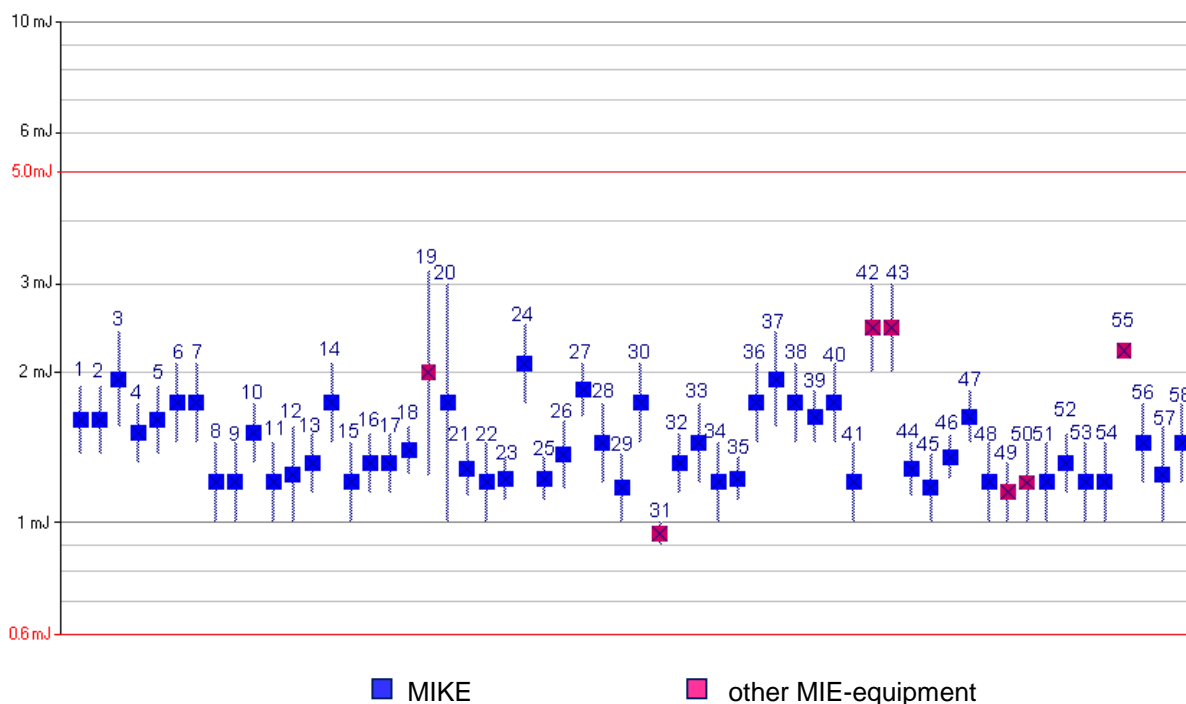

The individual results are drawn in chronological sequence (number of certificate).

3.1 Test procedure:

The method for determination of the MIE is described in the „Manual CaRo 13“.

3.2 Estimation of the statistical energy (Es):

The minimum ignition energy MIE lies, by definition, between two energy values:

$$E_1 < \text{MIE} < E_2$$

For the purpose of comparison between different apparatus, only one MIE value (Es) instead of the energy range (E1, E2) shall be used. This single value (Es) can be estimated by use of the probability of ignition as follows (EN 13821):

Provided that for the energy E2 a minimum of 5 dust concentrations evenly distributed are tested, the position of the MIE in the E1-E2 range can be estimated. At ignition energy E2, the number of dust concentrations with ignition, is divided by the total number of dust concentrations tested.

$$E_S = 10^{\log E_2 - \frac{I[E_2] \cdot (\log E_2 - \log E_1)}{(NI + 1) \cdot [E_2] + 1}}$$

where is: $I[E_2]$ = number of tests with ignition at the energy E2.
 $(NI+1)[E_2]$ = total number of tests at the energy E2.

3.3 Criteria for conformity:

Conformity between two equipment (a, b) is given, when the Es-values differ less than a factor of 3 (EN 13821).

$$1/3 < E_s(a) / E_s(b) < 3$$

Accordingly:


Conformity in the CaRo 13 is given, when the Es-value of each equipment differ less than a factor of 3 to the mean (Es) of all equipment:

Es / 3	Es	Es • 3
0.5 mJ	1.5 mJ	4.5 mJ

4. Troubles with chemical igniters


4.1 Simex-Igniters

Simex sent some faulty igniters with pressure oscillations. Pressure oscillations increase the turbulence and therefore the Kmax-value. Through the superimposed oscillation, the automatic evaluation is influenced or even wrong, which means the tangent has to be evaluated manually. The behaviour of the igniters is strongly variable from one production lot to another. Igniters with superimposed oscillations will give false results. In that case contact the manufacturer of the igniters.

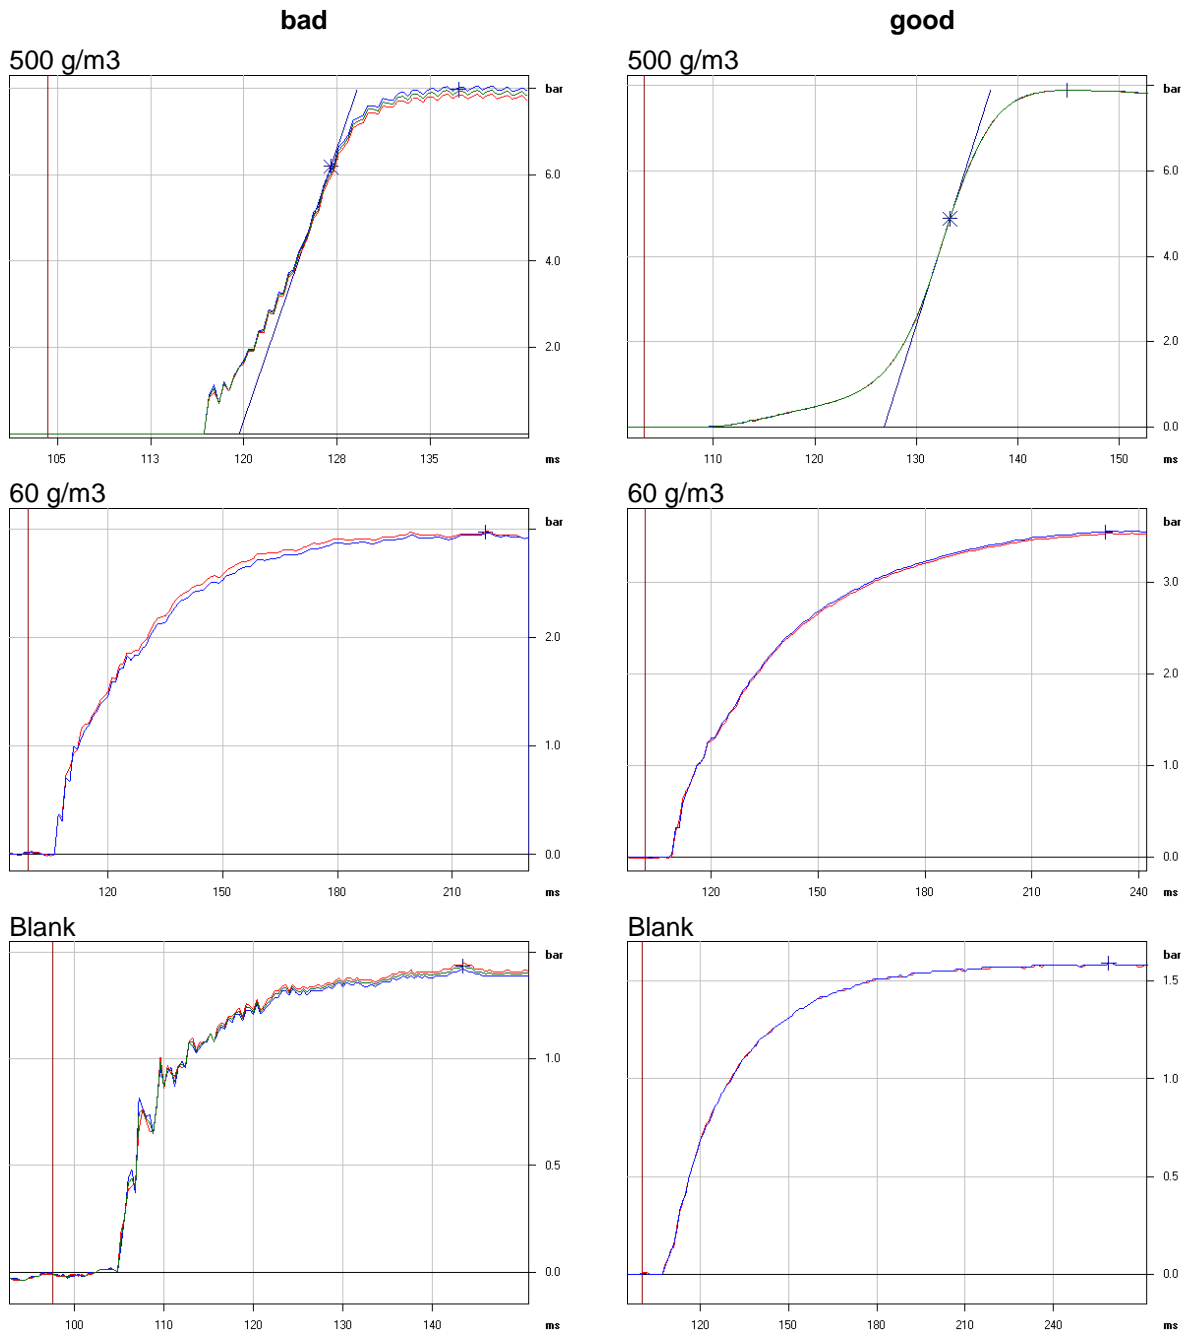

4.2 Sobbe-Igniters

Sobbe sent some faulty igniters with pressure oscillations. Pressure oscillations increase the turbulence and therefore the Kmax-value. Through the superimposed oscillation, the automatic evaluation is influenced or even wrong, which means the tangent has to be evaluated manually. The behaviour of the igniters is strongly variable from one production lot to another. Igniters with superimposed oscillations and/or casings that shattered will give false results. In that case contact the manufacturer of the igniters.

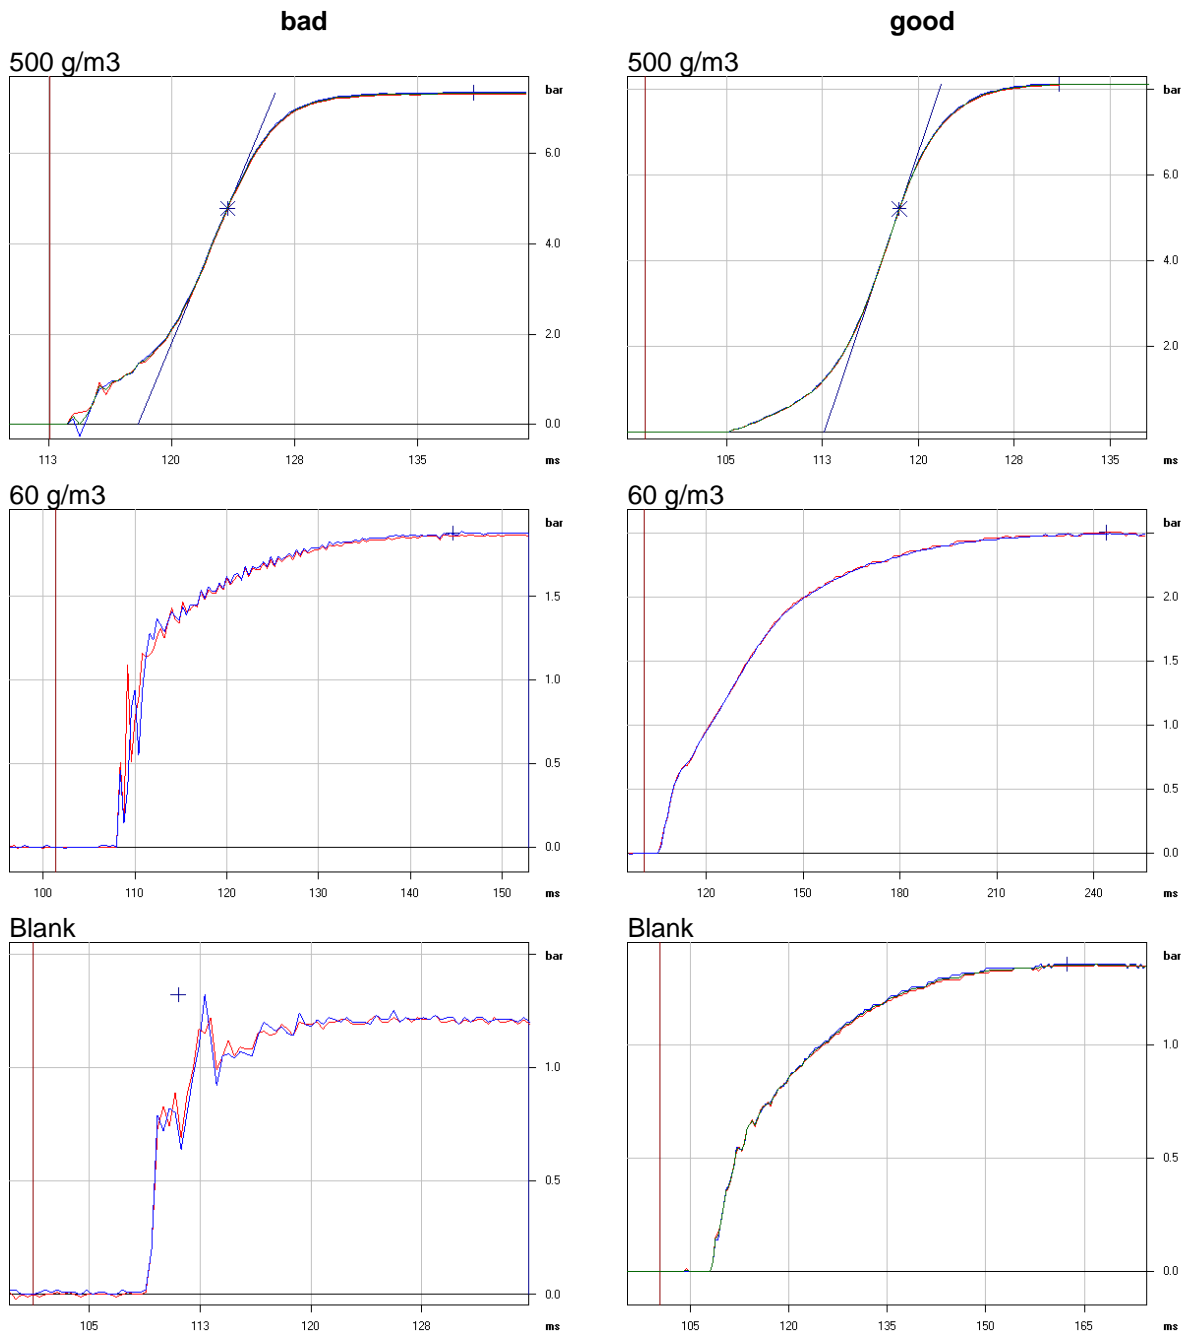

5. List of Participants

Country	Company Laboratory	E-Mail	Pmax Kmax	MIE
Australia	SIMTARS	fiona.clarkson@simtars.com.au	✓	✓
Australia	Workcover Londonderry Occ. Safety	david.pearson@workcover.nsw.gov.au	✓	
Austria	AUVA Abt. Unfallverhütung	nagy@auva.at	✓	✓
Austria	FireX Greßlehner GmbH	dietmar.gresslehner@firex.at	✓	
Austria	Montanuniversität Leoben	thomas.ehgartner@unileoben.ac.at	✓	✓
Belgium	ADINEX N.V.	frederik.norman@adinex.be	✓	✓
Canada	DalTech, Dalhouse University	paul.amyotte@dal.ca	✓	✓
Czechoslovakia	V V U U, a.s	mokosl@vuuu.cz	✓	✓
England	BRE Global	amendtl@bre.co.uk	✓	✓
England	Chilworth Technology Ltd	pbremble@chilworth.co.uk	✓	✓
France	INERIS	agnes.janes@ineris.fr	✓	✓
France	Rhodia Recherches & Technologies	noel.michel@solvay.com	✓	✓
Germany	AQura GmbH	klaus.budde@aqura.de		✓
Germany	BAM	mike.wappler@bam.de	✓	✓
Germany	BASF SE	johannes.a.fischer@basf.com	✓	✓
Germany	Bayer Technology	heinz-peter.keldenich@bayer.com	✓	✓
Germany	BGN	h.wolf.bgn@t-online.de	✓	✓
Germany	Boehringer Ingelheim Pharma	juergen.leininger@ing.boehringer- ingelheim.com	✓	✓
Germany	consilab	stephan.dreisch@consilab.de	✓	✓
Germany	DEKRA EXAM GmbH	matthias-reinecke@dekra.com	✓	✓
Germany	DGUV - IFA St. Augustin	sascha.hohmann@dguv.de	✓	
Germany	Henkel AG & Co.KGaA	michaela.berchter@henkel.com	✓	✓
Germany	Hochschule Mannheim	w.schmitt@hs-mannheim.de	✓	✓

Country	Company Laboratory	E-Mail	Pmax Kmax	MIE
Germany	IBExU GmbH	f.flemming@ibexu.de	✓	✓
Germany	INBUREX Consulting GmbH	martin.gosewinkel@inburex.com		✓
Germany	Sanofi-Aventis Deutschland GmbH	oe-labconsumables@sanofi-aventis.com		✓
Germany	Siemens AG	michael.nau@siemens.com	✓	✓
Germany	Wacker Chemie AG	alfred.augsberger@wacker.com	✓	✓
Hungary	Chemical Works of Gedeon Richter	bodnarr@richter.hu		✓
India	Intertek India Private Ltd.	ganeshkumar.janardhan@intertek.com		✓
Italy	INNOVHUB Divisione Stazione	mazzei@ssc.it	✓	✓
Italy	REDOX snc	info@labredox.com	✓	✓
Japan	Sumitomo Chemical Co., LTD	nishimarui@sc.sumitomo-chem.co.jp	✓	✓
Japan	TIIS - Technology Institution	matsuda@ankyo.or.jp		✓
Netherlands	Akzo Nobel	albert.colomer@akzonobel.com	✓	✓
Norway	GexCon AS	jth@gexcon.com	✓	✓
Poland	Central Mining Institute	zdyduch@gig.katowice.pl	✓	✓
Poland	CNBOP-PIB	mgrabarczyk@cnbop.pl	✓	✓
Slovenia	Sanolabor d.d	darko.kogoj@sanolabor.si	✓	
South Africa	CSIR Kloppersbos	lmthombe@csir.co.za	✓	
Switzerland	DSM Nutritional Products AG	romeo.isner@dsm.com		✓
Switzerland	F.HOFFMANN-LA ROCHE AG	klaus.schwenzfeuer@roche.com		✓
Switzerland	Firmenich SA	nicolas.dubois@fimenich.com	✓	
Switzerland	SWISSI Process Safety GmbH	adrien.bisel@swissi.ch	✓	✓

Country	Company Laboratory	E-Mail	Pmax Kmax	MIE
U.S.A	Chilworth Technology Inc.	dchurchwell@chilworthglobal.com	✓	
U.S.A	CYTEC Industries Inc.	mark.ryan@cytc.com	✓	✓
U.S.A	EMSL Analytical, Inc.	emirica@emsl.com	✓	✓
U.S.A	Exponent, Inc.	tmyers@exponent.com	✓	
U.S.A	FAUSKE & ASSOCIATES, LLC	dastidar@fauske.com	✓	✓
U.S.A	Fike Corporation FPS	sheri.brown@fike.com		✓
U.S.A	Firmenich Inc.	peter.de.rege@firmenich.com	✓	✓
U.S.A	ioMosaic Corporation	gotdon.j.iokinetic@iomosaic.com	✓	✓
U.S.A	Kidde-Fenwal Inc.	kemi.sorinmade@kidde-fenweal.com	✓	
U.S.A	Merck Sharp & Dohme Corp.	michael_toth@merck.com	✓	✓
U.S.A	The Dow Chemical Company	cv mashuga@dow.com		✓